

Performance Evaluations of a Novel Prototype of High Frequency Non-Contact Power Transformer

Laknath Gamage[†], Manabu Ishitobi and Mutsuo Nakaoka

ABSTRACT

In this paper, a practical implementation to reduce leakage flux of a high-frequency inverter based non-contact type power transformer composed of EE-shape ferrite cores is presented for key technology of the next generation medical use X-ray CT scanner system. Design consideration for the unique structure of the non-contact power transformer with 900mm in diameter is also introduced. The complete non-contact transformer is actually arranged by several blocks of the magnetic circuit assembled by using 10 small EE shape cores with 120mm in length. It is experimentally and analytically discussed from a reduced leakage flux viewpoint related to its inductively coupling coefficient. A practical method to lower the leakage flux is described based on effective Copper-Sheet-Treatment placed on EE shape ferrite cores of magnetic circuit.

Keywords : Non-contact power transformer, EE shaped ferrite core assembly, Inductively Coupling coefficient, Copper-Sheet-treatment of magnetic circuit, High Frequency Inverter

1. Introduction

In general, conductive connecting terminals are widely required for transferring electric power to the secondary battery banks, super capacitor assembly, electric machines, lighting equipments and electronic appliance. However, because of inferior connection, water or dust, corrosion and electric shocks might occur where connectors or terminals are essential. Not only to overcome these problems but also to make use of some other advantages, several feasible developments on non-contact transformer type or inductively mutual coupling type power supply circuit and systems have been carried out from an application point of view. Those related studies and developments are more required and acceptable for a variety of power conditioning and processing converters applications such as battery chargers for artificial hearts multi-links^{[3],[4]}, conveyance vehicles^{[5],[1]} and the other

Table 1. A variety of Non-Contact Power Supply Systems.

Input	Output	Output Power	Application
15V 2.5A DC	12V 2A DC	24W	Artificial Heart ^[7]
125V 0.4A DC	12V 3A DC	36W	EV-Battery Charger ^[17]
33.2V 3.6A DC	48V 2A DC	96W	EV-Battery Charger ^[15]
60V 2A DC	5V 20A DC	100W	Artificial Heart ^[18]
190V 3.2A DC	300V 1.9A DC	558W	Electric-conveyer Charger ^[19]
14.3V 333.6A	120.4V 24.1A	2.5kW	Under water power delivery ^[20]
230V 16A	200V 16A DC	3.2kW	EV-Battery Charger ^[14]
200V 30A	230V 14A DC	3.3kW	EV-Battery Charger ^[4]
300V 67A DC	400V 45A DC	20kW	EV-Battery Charger ^[16]
800V 150A DC	800V 141A DC	113kW	EV Battery* Charger ^[2]

*With matching transformer

organs, electric vehicles^[2], robotics with aircraft-passenger entertainment power distribution equipments^[6] medical power electronics appliances^[7], consumer products^[8] and so forth. Table 1 indicates some concrete power application areas of non-contact inductively coupled power transmission systems^{[9][10]}. As great possibilities of these related power transmission-processing fields, there

Manuscript received October, 8 2003

Revised November. 30, 2003.

† Corresponding Author: laknath3@yahoo.co.jp

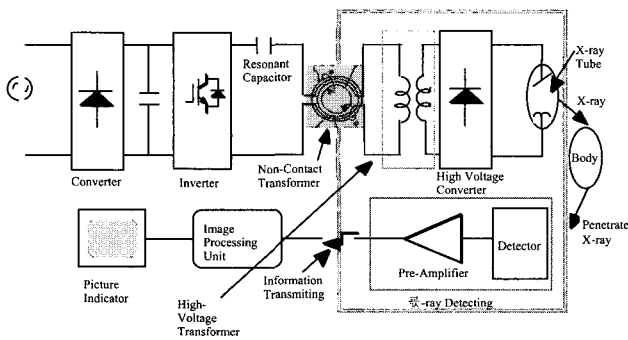


Fig. 1. CT Scanner System with Non-Contact Power Conversion Transformer.

are now hundreds of patents on non-contact power transmission systems, starting from Nicola Tesla's patent on electric railway system in 1892^[11]. On the contrary, only a few published papers are actually available in spite of a large number of patents^[12]. Of these, as far as the authors know, there are not any published research works on a non-contact power transmission and delivering system applied to a CT scanner system. The main reason for this is that the required feasible conditions cannot be achieved due to the large magnetizing current flow. In other words, due to the small magnetizing inductance, it gives a loose magnetic coupling coefficient to the non-contact power transformer of such a system mentioned above. This paper deals with a unique practical technique to magnify the coupling coefficient based on "Copper-treatment" of its magnetic circuit.

In this paper, a practical implementation to reduce leakage flux of a high-frequency resonant inverter based non-contact type power transformer composed of EE-shape ferrite cores is presented for key technology of the next generation medical use X-ray CT scanner system. Design considerations for the unique structure of the non-contact power transformer (900mm in diameter) for the power delivery system, are also introduced. In this paper, part of the whole non-contact transformer, designed for 120mm in length is designed and arranged by 10 small EE shape cores which is analytically and experimentally discussed and evaluated from the reducing leakage flux viewpoint related to the inductively coupling coefficient. The practical method to lowered the leakage flux is described and discussed on the basis of effective Copper-Sheet-Treatment placed on the EE shape ferrite cores as the magnetic circuit.

2. Non-contact high frequency power transformer and X ray CT scanner system

The developments of advanced medical power electronics technology required for high speed operation of X-ray CT scanner, have attracted special interest for introducing non-contact power transmission transformers instead of slip-rings used commonly in conventional^[13] X-ray CT scanners to deliver the electric power from the stationary part to the rotary part.

In general, magnetic inductive coupling in non contact transformer is the most important design factor in realization of a non-contact power transmission and delivering system. Therefore, the authors have focused upon the main research and development topics on the coupling coefficient of a non-contact power transformer incorporated into an X-ray CT scanner for medical use. An X-ray CT scanner system configuration with the non-contact power transmission transformer is schematically demonstrated in Fig. 1; and a detailed system configuration of the non-contact power transformer to be connected to a high-frequency inverter is illustrated in Fig. 2. This structure of the most essential non-contact power transformer is quite different from the other non-contact power supplying systems which have been discussed so far. That is because, the secondary side of the non-contact transformer in an X-ray CT scanner equipment can rotate and the high-frequency non contact transformer size is relatively large since a human body has to enter in to this rotating non contact high-frequency transformer for medical X-ray imaging diagnosis. As the secondary side of non contact transformer is usually rotating, the high-frequency non contact power transformer is designed so as to be symmetrical. Therefore, using a non-contact transformer of O-O type(That is ring type) magnetic coupling cores make best fitting for this kind of power processing system. Since the diameter of a core is practically 900mm as shown in Fig. 2, it is difficult to craft such a big core out of one lump of ferrite. Even though it is possible, the cost could be very high for practical implementation. Therefore, the authors propose small EE type ferrite cores assembly as illustrated on Fig. 2, that can cheaply be purchased on the market to fabricate the magnetic circuit of the unique high-frequency non-contact power transformer.

In experiment, the authors have build 3kW power level

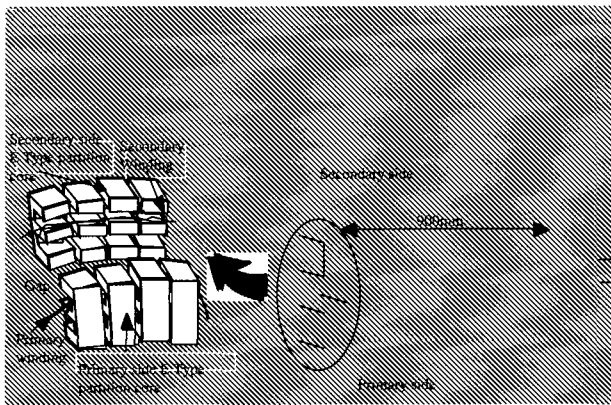


Fig. 2. Detailed Non-Contact Power Conversion Transformer.

setup with high efficiency. It is difficult to meet more than 3kW as output power rating, due to the drastic increase of excitation current in non-contact transformer with a small magnetizing inductance. The large leakage flux at the air gap of non-contact power transformer is the reason for this. Our main research aim is to develop only the non-contact

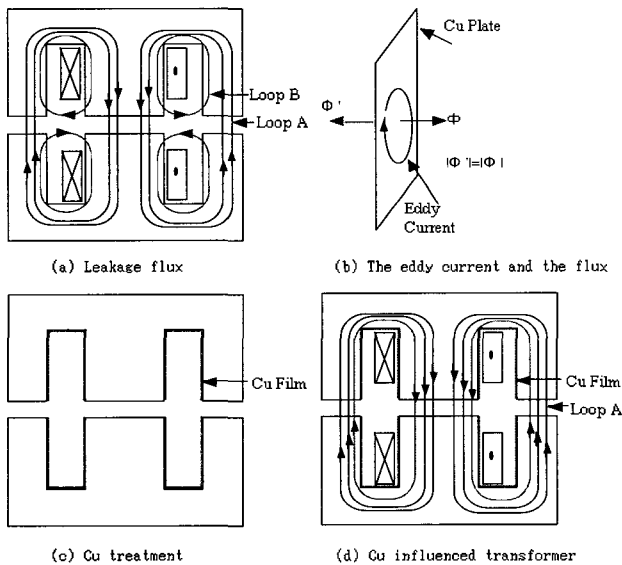


Fig. 3. The Copper-treatment at Ferite EE Core of Non-Contact Power Supply Transformer.

power transmission transformer of the proposed X-ray CT scanner system on the basis of magnifying the coupling coefficient by introducing the innovative Copper-treatment approach of EE shape cores based magnetic circuit. The technical problem is discussed for the following items.

- (1) The influence of the air gap on the coupling coefficient of EE ferrite cores.
- (2) The influence of the Copper-treatment on EE ferrite

cores on coupling coefficient of the non-contact power transmission transformer.

3. Core assembly concept of Copper-treatment on EE shape cores based magnetic circuit

Since the flux leakage at the air gap of the non-contact power conversion transformer is unavoidable, the authors desire to stop other flux leakage in the sense of having a better coupling coefficient by placing a Copper thin film at the window frame of the non-contact power transmission transformer as shown in Fig. 3. Figure 3(a) illustrates that the leakage flux in the core window and Fig. 3(d) depicts the reduced leakage flux because of the Copper-treatment. For EE ferrite core shape, as can be seen in the Fig. 3(c), a Copper thin film produces eddy current that makes another flux against the leakage flux and the leakage flux can in principle, be conveniently eliminated as shown in the 3(b).

4. Experimental and Simulation Results

As can be seen in Fig. 4, the experimental results show that the coupling coefficient k of the non-contact power transmission transformer goes down in accordance with the air gap. In the case of high power applications a low coupling coefficient is troublesome for the required air gap.

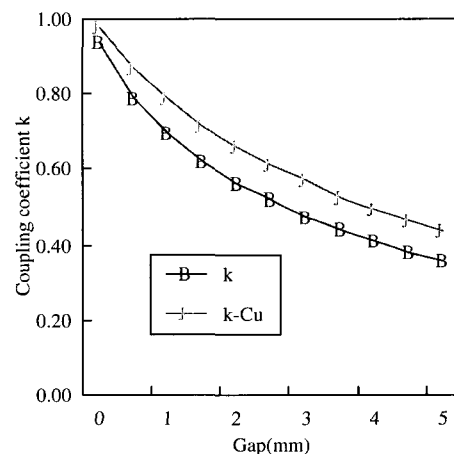


Fig. 4. Improvement of coupling coefficient in non-contact transformer.

At the same time, Fig. 4 depicts the coupling coefficient (k -Cu in the figure) of the non-contact power transmission transformer that is treated by a thin copper film is much higher than that of the normal non-contact power transmission transformer. The

results of magnetic analysis with MSC/Patran and ELF/Magic tools that use the integral element method also prove of this. For the analysis in this case, primary and secondary side cores of the non-contact power transmission transformer were divided into 698 small elements as shown in Fig. 5.

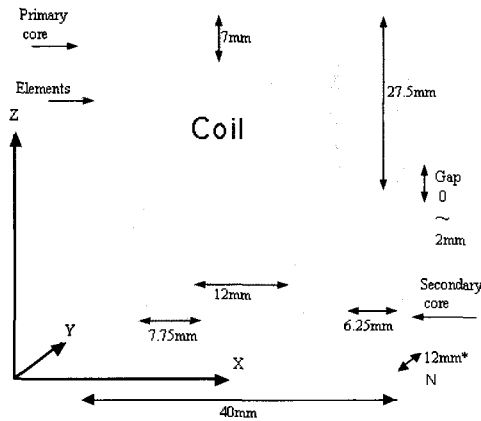


Fig. 5. EE type transformer model for magnetic field analysis.

The right hand side of the line in the middle of Fig.6, shows the secondary side of the non-contact power transmission transformer and the contrary is primary side of the non-contact power transmission transformer. From this analysis, it is noted that the flux density belongs to those elements depicted in Fig. 5. It is clear that the difference of the flux density varies with the place of the EE cores, but on the whole, the flux density is higher when the thin copper film in the core window frame or legs is present. However, the flux leakage of the air gap of the non-contact power transmission transformer can not be blocked by this copper treatment. As described above, the flux density of the EE shaped ferrite cores takes high values, after treating it on the basis of the thin copper film and therefore, the coupling coefficient of the non-contact power transmission transformer increases. It is proved that, according to experiment and simulation results, this thin copper film treatment is useful in improving the coupling coefficient of a non-contact transformer or an inductive coupler.

5. Ring Type Transformer with Small EE Shape Cores

The magnetic flux that leaking around the core is shown in Fig. 7(a), and the direction Z is the height direction of the EE shape ferrite cores. Large flux leakage can be seen in the region of the gap area, inside the core window. The arrow marks representing the vector of the leakage

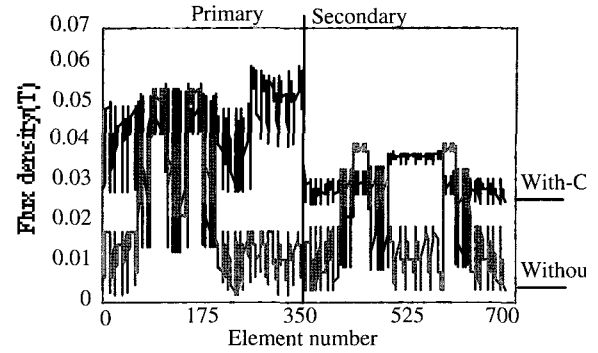


Fig. 6. Comparison of magnetic flux density when Copper-treatment applied to ferrite EE Core of non-contact Power Supply transformer.

flux. Fig. 7(b) depicts the flux density inside the core and the leakage flux around the core towards the Y direction,

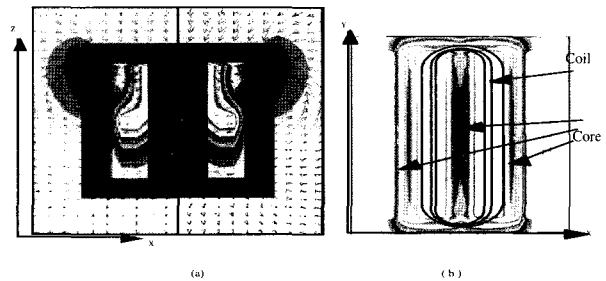


Fig. 7. Magnetic flux around the EE type transformer core.

where the next small type EE core to be fixed for manufacturing the large ring type non-contact power transmission transformer. As can be seen in the Fig. 7(b), fixed flux distribution has leaned towards the Y direction.

At the same time, to some extent, leakage flux can be seen at the end of the small non-contact power transmission transformer block. This amount can be neglected since it is not big enough to effect the neighboring small type transformers in the ring type non-contact power transmission transformer structure. Therefore it is possible to manufacture a large ring type non-contact power transmission transformer with the use of small type EE shaped cores that is cheap in the market.

6. Conclusions

The paper described a novel method to increase the magnetic coupling coefficient of a non-contact power transmission transformer. The actual efficiency in a non-contact power transmission transformer deteriorates with the air gap distance between the primary and the secondary sides of this non-contact transformer. This condition does not change even

after the Copper-treatment for EE shape ferrite core, explained in this paper. However, after this Copper-treatment, It is proved in experiment and simulations that the leakage flux of the non-contact power transmission transformer can be substantially reduced by applying the Copper-treatment on EE shape cores. As a result, the magnetic coupling coefficient of non-contact power transmission transformer goes up, effectively. At the same time it is capable of manufacturing a large ring type non-contact transformer with the use of small EE type ferrite cores that is cheap in the market.

References

- (1) Nishimura Toshihiro, Inoue Takeshi, Saito Masao and Nakaoka Mutsuo : "Energy Conversion System for Artificial Heart Using Resonant Type Soft-Switching Controlled DC-DC Converter", The Magnetic Society of Japan, Symposium & Technical Meeting Report(MAG-91-236), Vol. 91, No. 236, pp. 105-111 (1991).
- (2) Nasser H. Kutkut, Deepak M. Divan, Donald W. Novtny and Ray Marion: "Design Considerations and Topology Selection For a 120kW IGBT Converter for EV Fast Charging", Proceedings of 26th Annual IEEE Power Electronics Specialists Conference , pp. 238-244 (1995).
- (3) Atsuo Kawamura, Kazuaki Ishioka and Junzi Hirai: "Wireless Transmission of Power and Information through One High Frequency Current Resonant AC Link Inverter for Robot Servo Application", Technical report of the Institute of Electronics, Information and Communication Engineers , Vol. 95, No. 2, pp. 11-18 (1995).
- (4) Jacobus M. Barnard, Jan A Ferreira and Jacobus D. van Wyk: "Sliding Transformers for Linear Contactless Power Delivery", IEEE Transactions on Industrial Electronics , Vol. 44, No. 6, pp. 774-779 (1997).
- (5) Atsushi Okuno, Laknath Gamage and Mutsuo Nakaoka: "Performance Evaluations of High-Frequency Inverter-linked DC/DC Converter with Non-Contact Pickup Coil", IEEE Transaction on Industrial Electronics, Vol. 48, No. 2 pp. 475-477 (2001).
- (6) Arthur W. Kelley and William R. Owens: "Connectorless Power Supply for an Aircraft-Passenger Entertainment System", IEEE Transactions on Power Electronics, Vol. 4, No. 3, pp. 348-345 (1989).
- (7) C.W. Sherman, W.C. Clay, K.A. Dasse and B.D.T. Daly: "A Transcutaneous Energy Transmission(TET) System For High-Power Prosthetics", Proceedings of IEEE/Seventh Annual conference of the Engineering in Medicine and Biology Society, pp. 804-808 (1985).
- (8) Hideki Abe, Hiroshi Sakamoto and Koosuke Harada: "A Noncontact Charger Using a Resonant Converter with Parallel Capacitor of the Secondary Coil", IEEE Transactions on Industrial Applications, Vol. 36, No. 2, pp. 444-451 (2000).
- (9) Don A. G. Pedder, D. Brown, J. Andrew Skinner: "Contactless Electrical Energy Transmission system", IEEE Transactions on Industrial Electronics, Vol. 46, No. 1, pp. 23-30 (1999).
- (10) Robert L. Steigerwald, John A. Mallick and John N. Park: "Contactless Power Transfer System For a Rotational Load", United States Patent, No. 5,608,771 (1997).
- (11) Nicola Tesla: "Electric-Railway System", US Patent, No. 514972, (1892).
- (12) H.Takano, T.Hatakeyama, S.Sadamu, and T.Uchiyama: "X-ray CT System" Japanese patent, Publication number, 08-336521, JP 8336521 A (1996).
- (13) W. Taguchi, H. Fujimoto and T. Shinno, "Auklet Whole-Body Helical CT Scanner" Toshiba Review. Vol. 53, No. 1, pp. 13-20, 1998(Japanese).
- (14) X.Faubette, C.Rombaut, Ph. Le Moigne, A.Zcastelain, "A Battery Charger with Unity Power Factor for Electric Car "Proceedings of Power Electronics and Variable-Speed Drives, No. 399, pp.568-573, 1994.
- (15) Nasser H. Kutkut, Deepak M. Divan, Donald W. Novtny, "Inductive Charging Technologies for Electric Vehicles" Proceedings of IPEC, pp. 119-124, 1995.
- (16) K.Harada, F.Anan, K. Yamazaki, H. Sakamoto, K.sugimori, "Non-contact Charging for Electric Vehicles", Proceedings of Power Electronics and Motion Control Conference, Vol. 3, pp. 45-49, 1999.
- (17) Y. Jang and M. Jovanovic, "A New Soft-Switched Contactless Battery Charger with Robust Local Controllers", Proceedings of 25th International Telecommunications Energy Conference, Vol. 2, No. 3, pp. 473-479, 2003.
- (18) T. Nishimura, T.Inoue, M.Saito and M.Nakaoka, "Design of a Transcutaneous Energy Transmission System Employing a Zero-Voltage Switched Resonant Converter for Artificial Organs", Reports of Medical and Biological Engineering committee, MBE-91, No. 76 , pp. 1-4, 1991(Japanese).
- (19) A.W. Green and J.T.Boys, "10kHz Inductively Coupled Power Transfer Concept and Control", Proceedings of Power Electronics and Variable-Speed Drives, No. 399, pp. 694-699, 1994.
- (20) B.J. Heeres, D.W.Novotny, D.M.Divan and R.D.Lorenz, "Contactless Underwater Power Delivery" IEEE, Power Electronics Society, PESC 94.



Laknath Gamage was born in Yatiyantota, Sri Lanka. Received his MSc. degree in Electrical & Electronic Engineering from Graduate School of Science and Engineering, Yamaguchi University, Yamaguchi, Japan in 1998 and joined the division of Electrical Systems Engineering The Graduate School of Science and Engineering, Yamaguchi University, Yamaguchi Japan. He is working for APC Japan from 2001. His research interests include

High frequency resonant inverters, UPS systems and Non-contact power supply systems. He is a member of the Institute of Electrical Engineers of Japan and Japan Institute of Power Electronics.



Manabu Ishitobi was born in Shimane, Japan. Received his MSc. degree from Electrical & Electronic Engineering Graduate School of Science and Engineering, Yamaguchi University, Yamaguchi, Japan in 1998. He joined the division of Electrical Systems Engineering The Graduate School of Science and Engineering, Yamaguchi University, Yamaguchi Japan in 1998 and working towards his PhD now. His research interests include High frequency resonant inverters, DC-DC converters and Non-contact power supply systems. He is a member of the Institute of Electrical Engineers of Japan and Japan Institute of Power Electronics.



Mutsuo Nakaoka (Member) received his Dr-Eng. degree in Electrical Engineering from Osaka University, Osaka, Japan in 1981. He joined the Electrical and Electronics Engineering Department of Kobe University, Kobe, Japan in 1981. Since 1995, he has been a professor of the Electrical and Electronics Engineering Department, the Graduate School of Science and Engineering, Yamaguchi University, Yamaguchi, Japan. His research interests include application developments of power electronics circuit and systems. He received the 2001 premium paper award from IEE-UK, 2001/2003 IEEE-IECON Best Paper Award, the third paper award in IEEE-PEDS, 2003 IEEE-IAS James Melcher Prize Paper award and so on. He is now a chairman of IEEE Industrial Electronics Society Japan Chapter. Dr. Nakaoka is a member of the Institute of Electronics, Information and Communication Engineers of Japan, Institute of Illumination Engineering of Japan, European Power Electronics Association, the Japan Society of the Solar Energy, IEE-Korea and IEEE.