

Research Article



Micro-computed tomographic evaluation of the flow and filling ability of endodontic materials using different test models

Fernanda Ferrari Esteves Torres , Juliane Maria Guerreiro-Tanomaru ,
Gisselle Moraima Chavez-Andrade , Jader Camilo Pinto ,
Fábio Luiz Camargo Villela Berbert , Mario Tanomaru-Filho *

Department of Restorative Dentistry, São Paulo State University (UNESP), School of Dentistry, Araraquara, SP, Brazil



Received: Aug 14, 2019

Revised: Oct 16, 2019

Accepted: Nov 5, 2019

Torres FFE, Guerreiro-Tanomaru JM,
Chavez-Andrade GM, Pinto JC, Berbert FLCV,
Tanomaru-Filho M

*Correspondence to

Mario Tanomaru-Filho, DDS, PhD

Full Professor, Department of Restorative
Dentistry, São Paulo State University (UNESP),
School of Dentistry, Rua Humaitá, 1680, CEP
Araraquara, SP 14801-903, Brazil.
E-mail: tanomaru@uol.com.br

Copyright © 2020. The Korean Academy of
Conservative Dentistry
This is an Open Access article distributed
under the terms of the Creative Commons
Attribution Non-Commercial License ([https://
creativecommons.org/licenses/by-nc/4.0/](https://creativecommons.org/licenses/by-nc/4.0/))
which permits unrestricted non-commercial
use, distribution, and reproduction in any
medium, provided the original work is properly
cited.

Funding

This work was financed in part by the
Coordenação de Aperfeiçoamento de Pessoal
de Nível Superior, Brasil (CAPES) Finance
Code 001, and was fully supported by FAPESP
(2016/00321-0, 2017/19049-0).

Conflict of Interest

No potential conflict of interest relevant to this
article was reported.

ABSTRACT

Objectives: This study compared the flow and filling of several retrograde filling materials using new different test models.

Materials and Methods: Glass plates were manufactured with a central cavity and 4 grooves in the horizontal and vertical directions. Grooves with the dimensions used in the previous study ($1 \times 1 \times 2$ mm; length, width, and height respectively) were compared with grooves measuring $1 \times 1 \times 1$ and $1 \times 2 \times 1$ mm. Biodentine, intermediate restorative material (IRM), and mineral trioxide aggregate (MTA) were evaluated. Each material was placed in the central cavity, and then another glass plate and a metal weight were placed over the cement. The glass plate/material set was scanned using micro-computed tomography. Flow was calculated by linear measurements in the grooves. Central filling was calculated in the central cavity (mm^3) and lateral filling was measured up to 2 mm from the central cavity.

Results: Biodentine presented the least flow and better filling than IRM when evaluated in the $1 \times 1 \times 2$ model. In a comparison of the test models, MTA had the most flow in the $1 \times 1 \times 2$ model. All materials had lower lateral filling when the $1 \times 1 \times 2$ model was used.

Conclusions: Flow and filling were affected by the size of the test models. Higher grooves and materials with greater flow resulted in lower filling capacity. The test model measuring $1 \times 1 \times 2$ mm showed a better ability to differentiate among the materials.

Keywords: Dental materials; Endodontics; Methods; X-ray microtomography







INTRODUCTION

An ideal retrograde filling material should be resistant to dislocating forces [1,2] to prevent leakage between the root canal system and periradicular tissues [3]. Furthermore, the filling and sealing ability of endodontic cement can affect the long-term outcomes of endodontic surgery [4-6]. Root-end fillings with zinc oxide and eugenol-based cements, as well as calcium silicate-based materials, have shown a high probability of success [7,8]. However, the use of biomaterials has been proposed as a way to achieve more predictable outcomes [5-7,9].

Author Contributions

Conceptualization: Torres FFE, Tanomaru-Filho M, Guerreiro-Tanomaru JM; Data curation: Torres FFE, Pinto JC; Formal analysis: Torres FFE, Tanomaru-Filho M; Funding acquisition: Torres FFE, Tanomaru-Filho M; Investigation: Torres FFE, Tanomaru-Filho M, Chavez-Andrade GM; Methodology: Torres FFE, Chavez-Andrade GM; Project administration: Tanomaru-Filho M; Resources: Tanomaru-Filho M, Guerreiro-Tanomaru JM; Software: Torres FFE, Pinto JC; Supervision: Tanomaru-Filho M; Validation: Torres FFE, Tanomaru-Filho M, Berbert FLCV; Visualization: Torres FFE, Tanomaru-Filho M, Berbert FLCV; Writing - original draft: Torres FFE, Tanomaru-Filho M, Guerreiro-Tanomaru JM; Writing - review & editing: Tanomaru-Filho M, Torres FFE.

ORCID iDs

Fernanda Ferrari Esteves Torres 
<https://orcid.org/0000-0002-0631-3249>
 Juliane Maria Guerreiro-Tanomaru 
<https://orcid.org/0000-0003-0446-2037>
 Gisselle Moraima Chavez-Andrade 
<https://orcid.org/0000-0003-1394-2139>
 Jader Camilo Pinto 
<https://orcid.org/0000-0003-2023-1589>
 Fábio Luiz Camargo Villela Berbert 
<https://orcid.org/0000-0001-5230-0492>
 Mario Tanomaru-Filho 
<https://orcid.org/0000-0002-2574-4706>

The ability of endodontic materials to fill the spaces in the root canal in order to prevent fluid penetration is related to their flow [10]. However, flow and filling ability may not be directly proportional, considering that a material with a better ability to flow linearly will not necessarily provide greater filling capacity [11,12].

There are no previously established standards for evaluating the flow of root-end filling materials, and the International Standards Organization (ISO) standard [13] commonly used for the evaluation of root canal sealers does not document a correlation between the flow and fill properties of a material [12]. Thus, more accurate methods are required to evaluate the flow of endodontic materials [10]. For this reason, a novel test model was developed for concomitantly evaluating the flow and fill of endodontic cements using micro-computed tomography (CT) [12]. Micro-CT is a nondestructive, precise, and reproducible imaging tool that provides a 3-dimensional (3D) quantitative evaluation of filling materials [14].

The device developed to evaluate endodontic materials using micro-CT involves the delivery of endodontic cement between 2 glass plates with a metal weight over the top plate, with a similar design to that described in the ISO standards [13]. However, the bottom glass plate is manufactured with a central cavity and 4 grooves extending out horizontally and vertically. In this way, the model enables analysis of flow into the spaces and volumetric analysis, which allows the evaluation of the filling ability of a material in the central and lateral areas [12]. The proposed model using micro-CT assessment showed valid and reproducible results, and has the potential to improve flow analysis. Nevertheless, the influence of the size of the test models on the results has not yet been analyzed.

Since comparing different methods is essential for establishing the most suitable methodologies in endodontic research [15], the aim of this study was to investigate the influence of different sizes of test models on the linear flow and volumetric filling of Biodentine (Septodont, Saint-Maur-des-Fosses, France), intermediate restorative material (IRM; Dentsply DeTrey, Konstanz, Germany), and mineral trioxide aggregate (MTA; MTA-Angelus, Angelus, Londrina, PR, Brazil) using micro-CT. The null hypothesis was that there would be no differences in the flow and filling of the materials according to the test model used.

MATERIALS AND METHODS

Preparation of the test models

The first test model was manufactured according to the technique described by Tanomaru-Filho *et al.* [12]. A glass plate was fabricated with a central cavity (1 × 1 × 2 mm) (length, width, and height) and grooves extending out horizontally and vertically to the 4 sides. The other 2 dimensions were proposed to facilitate a comparison with the previous study, as follows: 1 × 1 × 1 mm and 1 × 2 × 1 (length, width, and height) (**Figure 1**). The samples

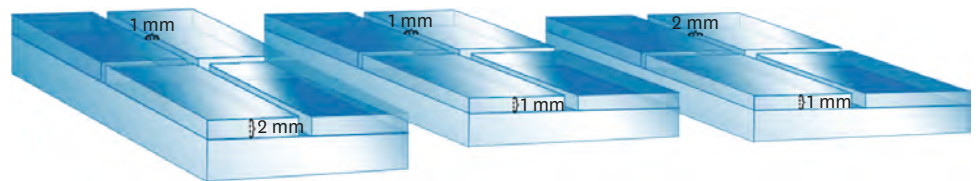


Figure 1. Illustration of the test models with a central cavity and lateral grooves manufactured with different dimensions: 1 × 1 × 2 mm, 1 × 1 × 1 mm, and 1 × 2 × 1 mm (length, width, and height).

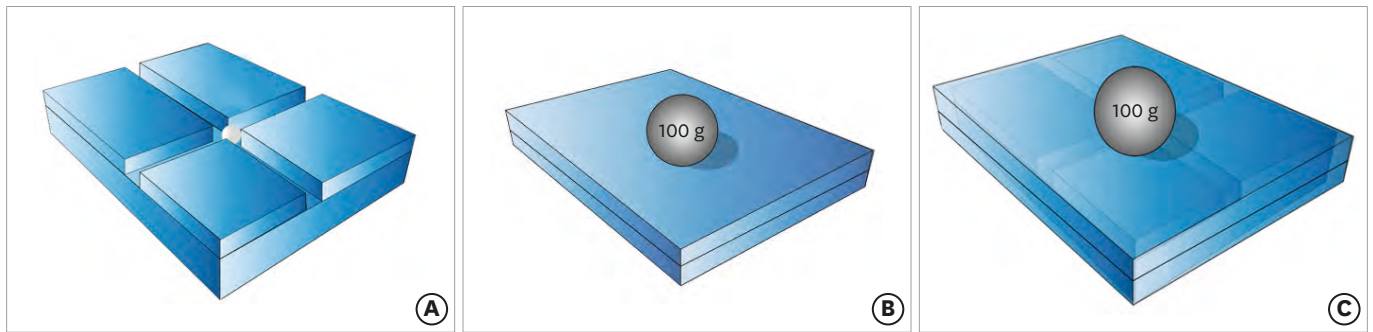


Figure 2. Illustration of the flow and filling ability evaluation process before the assessment using micro-computed tomography. The bottom glass plate with the endodontic cement placed in the central cavity (A). A view representing the assembled device, with the bottom glass plate, the top glass plate, and the metal weight over the cement (B). Another view representing the assembled device, using transparency to show the bottom plate and the metal weight over the material after flow inside the grooves (C).

were randomly divided into 3 groups ($n = 6$ each), according to the root-end filling material used. The complete information regarding the endodontic materials, their manufacturers, composition, and proportions is presented in **Table 1**. The procedure was performed by a single operator who was previously trained and calibrated. For each material, 0.050 mL was placed in the central cavity of the bottom glass plate, and another glass plate (20 g) and a metal weight (100 g) with a total mass of 120 g were placed on the materials and kept there for 10 minutes (**Figure 2**), according to the ISO 6876/2012 recommendation [13].

Micro-CT scanning and analysis

The glass plates/cement set was scanned with the SkyScan 1176 micro-CT system (SkyScan, Bruker, Kontich, Belgium). The micro-CT parameters were a voxel size of $9 \mu\text{m}$, 90 kVp, 278 mA, a 0.1 mm copper filter, and 360° scanning. The linear flow (mm) measurement of the material on each side of the grooves (horizontal and vertical) was analyzed. The mean of the 4 measurements was considered the linear flow for each evaluation. The volume (mm^3) filled by the material in the central area was determined as the central cavity filling. The volume (mm^3) filled by the materials in the lateral areas was determined up to 2 mm on each side of the central cavity. The mean of the 4 measurements was considered as the lateral cavity filling for each analysis. The data sets were reconstructed using NRecon software (V1.6.10.4, Bruker). The correction parameters for smoothing, beam hardening, and ring artefacts were defined for each material. The flow into the grooves and the filling of the central and lateral cavities were calculated using the CTAn software (V1.15.4.0, Bruker). CTAn was also used to create 3D models of the materials, which were visualized using the CTVol program (V2.3.1.0, Bruker).

Table 1. Endodontic materials, their manufacturers, their composition, and the proportions used

Material	Manufacturer	Composition	Proportion
Biodentine	Septodont, Saint-Maur-des-Fossés, France	Powder: tricalcium silicate, calcium carbonate, zirconium oxide, dicalcium silicate, calcium oxide, iron oxide Liquid: aqueous solution of a hydrosoluble polymer with calcium chloride	1 g of powder to 6 drops of liquid
IRM	Dentsply, Caulk Milford, DE, USA	Powder: zinc oxide, polymethyl methacrylate Liquid: eugenol, acetic acid	1 g of powder to 0.2 mL of liquid
MTA-Angelus	Angelus, Londrina, PR, Brazil	Powder: tricalcium silicate, dicalcium silicate, tricalcium aluminate, calcium oxide, bismuth oxide Liquid: distilled water	1 g of powder to 0.33 mL of distilled water

IRM, intermediate restorative material; MTA, mineral trioxide aggregate.

Table 2. Mean and standard deviation of the results of flow (mm) and filling (%) of endodontic materials evaluated in test models with different sizes (length, width, and height)

Factor	Biodentine	IRM	MTA
Linear flow (mm)			
1 × 1 × 1 mm	6.70 ± 0.94 ^{Aa}	7.19 ± 0.39 ^{Aa}	6.85 ± 0.11 ^{Ba}
1 × 2 × 1 mm	6.13 ± 0.98 ^{Aa}	6.86 ± 0.53 ^{Aa}	6.55 ± 0.34 ^{Ba}
1 × 1 × 2 mm	5.95 ± 0.76 ^{Ab}	7.41 ± 0.54 ^{Aa}	8.53 ± 1.01 ^{Aa}
Central filling (%)			
1 × 1 × 1 mm	92.38 ± 8.13 ^{Aa}	84.93 ± 7.72 ^{Aa}	87.75 ± 6.56 ^{Aa}
1 × 2 × 1 mm	88.23 ± 4.14 ^{Aa}	85.34 ± 9.09 ^{Aa}	87.65 ± 12.62 ^{ABa}
1 × 1 × 2 mm	79.92 ± 4.84 ^{Aa}	61.09 ± 5.25 ^{Bb}	71.53 ± 9.06 ^{Bab}
Lateral filling (%)			
1 × 1 × 1 mm	94.67 ± 4.48 ^{Aa}	80.59 ± 2.63 ^{Ab}	80.88 ± 6.39 ^{Ab}
1 × 2 × 1 mm	85.32 ± 11.37 ^{ABa}	78.62 ± 3.44 ^{Aa}	72.62 ± 7.66 ^{ABa}
1 × 1 × 2 mm	73.04 ± 8.37 ^{Ba}	56.63 ± 2.04 ^{Bb}	60.42 ± 5.26 ^{Bab}

The values are mean ± standard deviation. Different lowercase letters on the same line indicate statistically significant differences between the different cements ($p < 0.05$). Different capital letters in the same column indicate statistically significant differences between the different test models ($p < 0.05$) (2-way analysis of variance and Tukey test).

IRM, intermediate restorative material; MTA, mineral trioxide aggregate.

Statistical analysis

The normality of the data was tested using the Kolmogorov-Smirnov test. The statistical analysis was performed with 2-way analysis of variance and the Tukey parametric test with a significance level of 5%.

RESULTS

The results are presented in **Table 2**. MTA and IRM presented similar linear flow and central cavity filling in all test models ($p > 0.05$). MTA had greater flow when using the test model with a height of 2 mm, with a higher value than Biodentine ($p < 0.05$). For central cavity filling, IRM and MTA showed worse results in the model with a height of 2 mm than in the model measuring 1 × 1 × 1 mm ($p < 0.05$). The same occurred for lateral cavity filling in all materials ($p < 0.05$). Biodentine showed better filling than IRM in the model with a height of 2 mm ($p < 0.05$). The calculation of the filling of the materials in the central and lateral areas, as well as a 3D model illustrating the flow and filling of the materials into the grooves, can be seen in **Figure 3**.

DISCUSSION

The flowability of endodontic sealers is evaluated using the ISO 6876/2012 standard [13] because a proper flow may allow filling irregularities [16]. However, this conventional test does not allow a 3D assessment of the filling ability of a material. Thus, it is not possible to determine whether proper flow is associated with adequate filling. Moreover, there is no standard for assessing the flow of root-end filling cements. Therefore, we evaluated the flow and filling of root-end filling materials using micro-CT according to Tanomaru-Filho *et al.* [12]. According to the authors, volumetric data reflect the ability of a material to fill a space and to flow into lateral spaces, an important property for endodontic materials. Furthermore, the proposed device allowed standardization of the amount of cement and the pressure to be used on the material during the test, similar to the device described in the ISO standard [13].

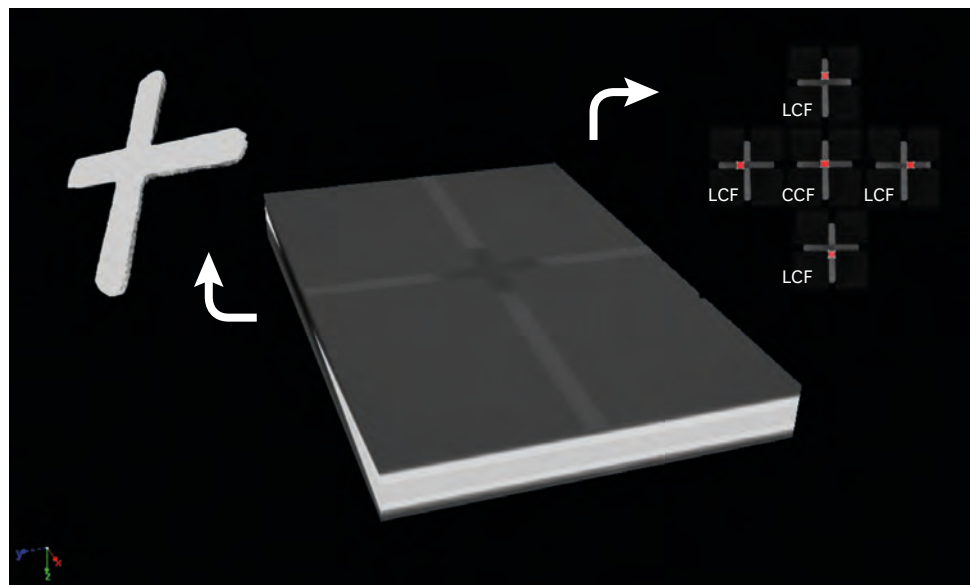


Figure 3. Illustration created in the CTvox software showing the assembled device composed of the bottom glass plate, the cement after flow inside the grooves, and the top glass plate during the scanning process on micro-computed tomography. The flow and filling representation were performed in 3 dimensions using the CTVol software. Central cavity filling (CCF) and lateral cavity filling (LCF) were evaluated using the CTAn software.

Numerous studies have proposed using micro-CT to complement conventional evaluations of endodontic materials [12,14,17-21]. However, since micro-CT is a relatively new methodology, these evaluations have lacked standardization. For this reason, it is necessary to evaluate the influence of the evaluation method on the results obtained.

Based on a new technique already recommended in the literature [12], the current study aimed to assess the influence of the dimensions of the test models on the flow and filling properties of different endodontic cements. Similar to previously observed results [11,12], there was no direct correlation between the properties evaluated, since when a material presented a greater flow, a proportional filling of the cavity was not observed. It was also found that the height of the test models had an influence on the results. When a height of 2 mm was used, MTA presented higher flow but less filling capacity. For Biodentine and IRM, lateral cavity filling was also lower when the highest model was used. In contrast, when the smallest dimensions were used, it was possible to observe greater flow and filling. These findings may be directly applied to clinical situations, as root canal systems present small irregularities to be filled by the material. Thus, our null hypothesis was rejected since the test models showed a direct influence on the results.

IRM is a zinc and eugenol-based cement that has been used for several decades. However, its cytotoxicity is an important limitation of this material [7]. Although Biodentine presents lower linear flow in the 2-mm-high model, it showed better filling than IRM. Therefore, it may be suggested that Biodentine has a better filling ability than IRM, which may be supported by previous results indicating that IRM showed high microleakage [22]. However, Tsesis *et al.* [23] evaluated the apical portion of root canals filled with MTA, IRM, and Biodentine regarding *Enterococcus faecalis* colonization and observed no differences among the root-end filling materials in the mean and maximal depths of bacterial colonization into the dentinal tubules. Those results suggest that similar success rates for root-end filling can be obtained using calcium silicate-based materials or cements based on zinc oxide and eugenol [8].

However, it is also important to consider that calcium silicate-based materials, such as MTA and Biodentine, are potentially bioactive when placed in direct contact with dentin, and may promote biomineralization [24]. This property enables a better seal for retrograde fillings [25], making them better options for the repair of furcal perforations [1]. Moreover, Akbulut *et al.* [26] observed no significant difference in the push-out bond strength of MTA-Angelus and Biodentine, in agreement with the similar characteristics observed for both materials in the present study.

Previous studies have evaluated the filling capacity of MTA and Biodentine using micro-CT [27-29]. This non-invasive imaging technique provides high-resolution images and enables a 3D volumetric analysis [30], allowing a material's filling ability to be evaluated in terms of the filling percentage [27,28]. Furthermore, the methodology employed in the current study allows a concomitant analysis of a material's flow rate and filling of lateral spaces [12], which is more difficult to achieve for root-end filling cements.

Regarding central cavity filling, our results showed that Biodentine and MTA presented similar values in all the test models. This finding corroborates the report of Küçükaya *et al.* [27], who observed no significant difference between the obturation quality of MTA and Biodentine in terms of percentage volume of filling materials on micro-CT. The authors used tooth models that simulated perforating internal root resorption in the middle third of the root, and observed that the apical portion of the specimens presented a lower percentage of filling materials than the resorption cavities. Their result agrees with the present study, where the percentage of filling in the central cavity was greater than in the lateral spaces.

It is important to emphasize that when using the test model with the smallest dimensions, Biodentine showed better lateral filling than MTA. This finding may be related to the smaller particle size and higher surface area of Biodentine when compared to MTA. Moreover, the Biodentine radiopacifier is zirconium oxide, which has a smaller particle size and allows less porosity than the bismuth oxide used in MTA-Angelus [31]. Therefore, many studies have stated that a major disadvantage of MTA is its handling properties and its granular consistency. Consequently, additives have been proposed to increase its plasticity. Among these additives, methylcellulose, calcium chloride, calcium lactate gluconate, and propylene glycol improved the handling of MTA [32-34]. In Biodentine, a hydro-soluble polymer is incorporated to enhance its handling properties [31].

A recent systematic review was undertaken in order to evaluate the influence of variation in the design of the push-out bond test in endodontic research [35]. The authors concluded that standardization is required for future research, as well as accurate reporting of all test variables, to assess the impact of specific designs on endodontic evaluations. This statement reinforces the importance of conducting studies to establish methods for the reliable analysis of material properties.

CONCLUSIONS

The linear flow and filling ability of materials were affected by the size of the evaluated test models. Higher grooves and materials with higher flow showed a lower filling capacity. The test model measuring $1 \times 1 \times 2$ mm showed the best ability to differentiate filling capacity among different materials.

ACKNOWLEDGEMENTS

The authors thank Renato Luiz Carvalho for his assistance with the illustrations.

REFERENCES

1. Adl A, Sadat Shojaee N, Pourhatami N. Evaluation of the dislodgement resistance of a new pozzolan-based cement (EndoSeal MTA) compared to ProRoot MTA and Biodentine in the presence and absence of blood. *Scanning* 2019;2019:3863069.
[PUBMED](#) | [CROSSREF](#)
2. Küçükkaya Eren S, Aksel H, Serper A. Effect of placement technique on the push-out bond strength of calcium-silicate based cements. *Dent Mater J* 2016;35:742-747.
[PUBMED](#) | [CROSSREF](#)
3. Parirokh M, Torabinejad M. Mineral trioxide aggregate: a comprehensive literature review--Part I: chemical, physical, and antibacterial properties. *J Endod* 2010;36:16-27.
[PUBMED](#) | [CROSSREF](#)
4. Alcalde MP, Vivian RR, Marciano MA, Duque JA, Fernandes SL, Rosseto MB, Duarte MA. Effect of ultrasonic agitation on push-out bond strength and adaptation of root-end filling materials. *Restor Dent Endod* 2018;43:e23.
[PUBMED](#) | [CROSSREF](#)
5. Küçükkaya Eren S, Parashos P. Adaptation of mineral trioxide aggregate to dentine walls compared with other root-end filling materials: a systematic review. *Aust Endod J* 2019;45:111-121.
[PUBMED](#) | [CROSSREF](#)
6. Saxena P, Gupta SK, Newaskar V. Biocompatibility of root-end filling materials: recent update. *Restor Dent Endod* 2013;38:119-127.
[PUBMED](#) | [CROSSREF](#)
7. Akbulut MB, Arpacı PU, Eldeniz AU. Effects of four novel root-end filling materials on the viability of periodontal ligament fibroblasts. *Restor Dent Endod* 2018;43:e24.
[PUBMED](#) | [CROSSREF](#)
8. Kohli MR, Berenji H, Setzer FC, Lee SM, Karabucak B. Outcome of endodontic surgery: a meta-analysis of the literature-part 3: comparison of endodontic microsurgical techniques with 2 different root-end filling materials. *J Endod* 2018;44:923-931.
[PUBMED](#) | [CROSSREF](#)
9. Al-Haddad A, Abu Kasim NH, Che Ab Aziz ZA. Interfacial adaptation and thickness of bioceramic-based root canal sealers. *Dent Mater J* 2015;34:516-521.
[PUBMED](#) | [CROSSREF](#)
10. Song YS, Choi Y, Lim MJ, Yu MK, Hong CU, Lee KW, Min KS. *In vitro* evaluation of a newly produced resin-based endodontic sealer. *Restor Dent Endod* 2016;41:189-195.
[PUBMED](#) | [CROSSREF](#)
11. Almeida JF, Gomes BP, Ferraz CC, Souza-Filho FJ, Zaia AA. Filling of artificial lateral canals and microleakage and flow of five endodontic sealers. *Int Endod J* 2007;40:692-699.
[PUBMED](#) | [CROSSREF](#)
12. Tanomaru-Filho M, Torres FF, Bosso-Martelo R, Chávez-Andrade GM, Bonetti-Filho I, Guerreiro-Tanomaru JM. A novel model for evaluating the flow of endodontic materials using micro-computed tomography. *J Endod* 2017;43:796-800.
[PUBMED](#) | [CROSSREF](#)
13. International Organization for Standardization. ISO 6876: Dental root canal sealing materials. Geneva: International Organization for Standardization; 2012.
14. Kim K, Kim DV, Kim SY, Yang S. A micro-computed tomographic study of remaining filling materials of two bioceramic sealers and epoxy resin sealer after retreatment. *Restor Dent Endod* 2019;44:e18.
[PUBMED](#) | [CROSSREF](#)
15. Jang JH, Lee HW, Cho KM, Shin HW, Kang MK, Park SH, Kim E. *In vitro* characterization of human dental pulp stem cells isolated by three different methods. *Restor Dent Endod* 2016;41:283-295.
[PUBMED](#) | [CROSSREF](#)
16. Duarte MA, Ordinola-Zapata R, Bernardes RA, Bramante CM, Bernardineli N, Garcia RB, de Moraes IG. Influence of calcium hydroxide association on the physical properties of AH Plus. *J Endod* 2010;36:1048-1051.
[PUBMED](#) | [CROSSREF](#)

17. Kim J, Song YS, Min KS, Kim SH, Koh JT, Lee BN, Chang HS, Hwang IN, Oh WM, Hwang YC. Evaluation of reparative dentin formation of ProRoot MTA, Biodentine and BioAggregate using micro-CT and immunohistochemistry. *Restor Dent Endod* 2016;41:29-36.
[PUBMED](#) | [CROSSREF](#)
18. Oltra E, Cox TC, LaCourse MR, Johnson JD, Paranjpe A. Retreatability of two endodontic sealers, EndoSequence BC Sealer and AH Plus: a micro-computed tomographic comparison. *Restor Dent Endod* 2017;42:19-26.
[PUBMED](#) | [CROSSREF](#)
19. Torres FF, Guerreiro-Tanomaru JM, Bosso-Martelo R, Chavez-Andrade GM, Tanomaru Filho M. Solubility, porosity and fluid uptake of calcium silicate-based cements. *J Appl Oral Sci* 2018;26:e20170465.
[PUBMED](#) | [CROSSREF](#)
20. Torres FF, Guerreiro-Tanomaru JM, Bosso-Martelo R, Espir CG, Camilleri J, Tanomaru-Filho M. Solubility, porosity, dimensional and volumetric change of endodontic sealers. *Braz Dent J* 2019;30:368-373.
[PUBMED](#) | [CROSSREF](#)
21. Yanpiset K, Banomyong D, Chotvorarak K, Srisatjaluk RL. Bacterial leakage and micro-computed tomography evaluation in round-shaped canals obturated with bioceramic cone and sealer using matched single cone technique. *Restor Dent Endod* 2018;43:e30.
[PUBMED](#) | [CROSSREF](#)
22. Peralta SL, Leles SB, Dutra AL, Guimarães VB, Piva E, Lund RG. Evaluation of physical-mechanical properties, antibacterial effect, and cytotoxicity of temporary restorative materials. *J Appl Oral Sci* 2018;26:e20170562.
[PUBMED](#) | [CROSSREF](#)
23. Tsesis I, Elbahary S, Venezia NB, Rosen E. Bacterial colonization in the apical part of extracted human teeth following root-end resection and filling: a confocal laser scanning microscopy study. *Clin Oral Investig* 2018;22:267-274.
[PUBMED](#) | [CROSSREF](#)
24. Aksel H, Küçükaya Eren S, Askerbeyli Örs S, Karaismailoğlu E. Surface and vertical dimensional changes of mineral trioxide aggregate and biodentine in different environmental conditions. *J Appl Oral Sci* 2018;27:e20180093.
[PUBMED](#) | [CROSSREF](#)
25. Biočanin V, Antonijević Đ, Poštić S, Ilić D, Vuković Z, Milić M, Fan Y, Li Z, Brković B, Đurić M. Marginal gaps between 2 calcium silicate and glass ionomer cements and apical root dentin. *J Endod* 2018;44:816-821.
[PUBMED](#) | [CROSSREF](#)
26. Akbulut MB, Bozkurt DA, Terlemez A, Akman M. The push-out bond strength of BIOfactor mineral trioxide aggregate, a novel root repair material. *Restor Dent Endod* 2019;44:e5.
[PUBMED](#) | [CROSSREF](#)
27. Küçükaya Eren S, Aksel H, Askerbeyli Örs S, Serper A, Koçak Y, Ocak M, Çelik HH. Obturation quality of calcium silicate-based cements placed with different techniques in teeth with perforating internal root resorption: a micro-computed tomographic study. *Clin Oral Investig* 2019;23:805-811.
[PUBMED](#) | [CROSSREF](#)
28. Torres FF, Bosso-Martelo R, Espir CG, Cirelli JA, Guerreiro-Tanomaru JM, Tanomaru-Filho M. Evaluation of physicochemical properties of root-end filling materials using conventional and Micro-CT tests. *J Appl Oral Sci* 2017;25:374-380.
[PUBMED](#) | [CROSSREF](#)
29. Tang JJ, Shen ZS, Qin W, Lin Z. A comparison of the sealing abilities between Biodentine and MTA as root-end filling materials and their effects on bone healing in dogs after periradicular surgery. *J Appl Oral Sci* 2019;27:e20180693.
[PUBMED](#) | [CROSSREF](#)
30. Yilmaz A, Helvacioğlu-Yigit D, Gur C, Ersev H, Kiziltas Sendur G, Avcu E, Baydemir C, Abbott PV. Evaluation of dentin defect formation during retreatment with hand and rotary instruments: a micro-CT study. *Scanning* 2017;2017:4868603.
[PUBMED](#) | [CROSSREF](#)
31. Camilleri J, Sorrentino F, Damidot D. Investigation of the hydration and bioactivity of radiopacified tricalcium silicate cement, Biodentine and MTA Angelus. *Dent Mater* 2013;29:580-593.
[PUBMED](#) | [CROSSREF](#)
32. Ber BS, Hatton JF, Stewart GP. Chemical modification of proroot mta to improve handling characteristics and decrease setting time. *J Endod* 2007;33:1231-1234.
[PUBMED](#) | [CROSSREF](#)

33. Hsieh SC, Teng NC, Lin YC, Lee PY, Ji DY, Chen CC, Ke ES, Lee SY, Yang JC. A novel accelerator for improving the handling properties of dental filling materials. *J Endod* 2009;35:1292-1295.
[PUBMED](#) | [CROSSREF](#)
34. Duarte MA, Alves de Aguiar K, Zeferino MA, Vivan RR, Ordinola-Zapata R, Tanomaru-Filho M, Weckwerth PH, Kuga MC. Evaluation of the propylene glycol association on some physical and chemical properties of mineral trioxide aggregate. *Int Endod J* 2012;45:565-570.
[PUBMED](#) | [CROSSREF](#)
35. Brichko J, Burrow MF, Parashos P. Design variability of the push-out bond test in endodontic research: a systematic review. *J Endod* 2018;44:1237-1245.
[PUBMED](#) | [CROSSREF](#)